



Instructions For Use BBS-1-IFU

Rev. Date: Dec. 3, 2012

Revision: 2

Page 1 of 2

P.O. Box 3286 - Logan, Utah 84323, U.S.A. - Tel. (800) 729-8350 – Tel. (435) 755-9848 - Fax (435) 755-0015 - www.scytek.com

Gram Stain Kit (Modified Brown & Brenn)


Description: The Gram Stain Kit (Modified Brown & Brenn) is intended for the demonstration and differentiation of Gram-positive and Gram-negative bacteria.

Gram Positive Bacteria: Blue
Gram Negative Bacteria: Red
Other Tissue: Slightly Yellow - Pink
Nuclei: Red

Uses/Limitations: Not to be taken internally.
For In-Vitro Diagnostic use only.
Histological applications.
Do not use if reagents become cloudy.
Do not use past expiration date.
Use caution when handling reagents.
Non-Sterile.

Control Tissue: Any well fixed tissue section.
Air dried smear.

Ordering Information and Current Pricing at www.scytek.com

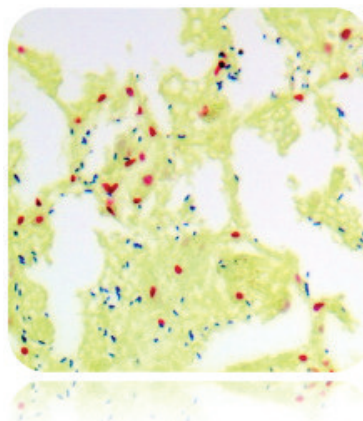

Kit Contents:

<u>Item #</u>	<u>Product Name</u>	<u>Volume</u>	<u>Storage</u>
GVS125	Gentian Violet Solution	125 ml	18-25°C
LIS125	Lugol's Iodine Solution	125 ml	18-25°C
GDS125	Gram's Decolorizer Solution	125 ml	18-25°C
SOH125	Safranin O Solution	125 ml	18-25°C
PAB125	Picric Acid - Acetone Solution (0.1%)	125 ml	18-25°C

Precautions: Keep away from open flame.
Avoid contact with skin and eyes.
Harmful if swallowed.
Follow all Federal, State, and local regulations regarding disposal.

Storage: 18° C



25° C



ScyTek Laboratories, Inc.
205 South 600 West
Logan, UT 84321
U.S.A.



EC REP EmergoEurope (31)(0) 70 345-8570
Molsnstraat 15
2513 BH Hague, The Netherlands

Procedure (Standard):

1. Deparaffinize sections if necessary and hydrate to distilled water.
2. Cover tissue section with Gentian Violet Solution and incubate for 2 minutes.
3. Rinse slide in distilled water to remove excess stain.
4. Cover tissue section with Lugol's Iodine Solution and incubate for 1 minute.
5. Rinse slide in running tap water to remove excess iodine.
6. Dip 1 time in distilled water.
7. Apply Gram's Decolorizer dropwise or by repeated dips until color no longer bleeds off section.
8. Rinse slide quickly in distilled water (2-5 seconds).
9. Cover tissue section with Safranin O Solution and incubate for 4 minutes.
10. Rinse slide quickly in distilled water to remove excess stain.
11. Dip once in absolute alcohol and blot dry.
12. Cover tissue section with Picric Acid - Acetone Solution (0.1%) and incubate with agitation for 2-10 seconds.
13. Dehydrate slide very quickly in 3 changes of absolute alcohol.
14. Clear in 2 changes of xylene or xylene substitute, and mount in synthetic resin.

References:

1. Isenberg, H.H. Clinical Microbiology Procedures Handbook. American Society for Microbiology, 1992.
2. Sheehan, DC., Hrapchak, BB. Theory and Practice of Histotechnology; 1980, page 235.
3. Brown, J.H., Brenn, L. A method for the differential staining of gram-positive and gram-negative bacteria in tissue sections. Bulletin Johns Hopkins Hospital, 1931, Volume 48, pages 69-73.
4. Gram, C. Forstchr. Med., Volume 2, page 185, 1884.

Bulk Reagent Ordering Information and Current Pricing at www.scytek.com

Description:	Catalog #	Volume
Gentian Violet Solution	GVS125	125 ml
	GVS500	500 ml
	GVS999	1000 ml
Lugol's Iodine Solution	LIS125	125 ml
	LIS500	500 ml
	LIS999	1000 ml
Gram's Decolorizer	GDS125	125 ml
	GDS500	500 ml
	GDS999	1000ml
Safranin O Solution	SOH125	125 ml
	SOH500	500 ml
	SOH999	1000 ml
Picric Acid – Acetone Solution (0.1%)	PAB125	125 ml
	PAB500	500 ml
	PAB999	1000 ml

Storage: 18° C



25° C



ScyTek Laboratories, Inc.
205 South 600 West
Logan, UT 84321
U.S.A.



EC REP EmergoEurope (31)(0) 70 345-8570
Molsstraat 15
2513 BH Hague, The Netherlands